

Adaptive Neural Network Imaging in Medical Systems

Constantinos S. Pattichis^{1,2}, Marios S. Pattichis²

¹Department of Computer Science, University of Cyprus, Kallipoleos 75,
P.O. Box 20537, CY1678 Nicosia, Cyprus email: pattichi@ucy.ac.cy

²Department of Electrical and Computer Engineering, University of New Mexico,
Albuquerque, NM 87131-1356, USA email: pattichis@ece.unm.edu

Abstract

Recent technological advances in medicine facilitated the development of sophisticated equipment enabling the better delivery of health care services. In parallel, artificial neural networks emerged as promising tools for the application and implementation of intelligent systems. The aim of this paper is to provide a snapshot of the application of neural network systems in medical imaging. The paper will highlight neural network applications in the analysis of cervicovaginal smears, mammography, microscopy, ultrasound imaging, and lesion placement in pallidotomy. It is anticipated that the application of neural network systems in medicine will provide the framework for the development of emerging medical systems, enabling the better delivery of health care.

I. Introduction

The overall objective of Computer Aided Diagnostic (CAD) systems is to enable the early diagnosis, disease monitoring, and better treatment. The advantages of CAD systems can be summarized as follows: *Standardization.* Diagnoses obtained from different laboratories using similar criteria can be verified. *Sensitivity.* Findings on a particular subject may be compared with a database of normal values and/or a decision can be made by a CAD system deciding whether or not an abnormality exists. *Specificity.* Findings may be compared with databases for various diseases and/or a decision can be made by the CAD system with respect to the type of abnormality. *Equivalence.* Results from a series of examinations of the same patient may be compared to decide whether there is evidence of disease progression or of response to treatment. In addition, the findings of different CAD systems can be compared to determine which are more sensitive and specific. *Efficacy.* The results of different treatments can be more properly evaluated. Medical imaging provides vital information for CAD systems.

The objective of this paper is to present a snapshot of adaptive neural network applications in medical imaging and how these techniques can be integrated in CAD systems.

According to Widrow and Stearns [1], the major characteristics of an adaptive system can be summarized as follows: 1. They can automatically adapt (self-optimize) in the face of changing (nonstationary) environments and changing system requirements. 2. They can be trained to perform specific filtering and decision-making tasks. 3. They can extrapolate a model of behavior to deal with new situations after having been trained on a finite and often small number of training signals or patterns. 4. To a limited extent, they can repair themselves; that is, they can adapt around certain kinds of internal defects. 5. They can usually be described as nonlinear systems with time-varying parameters. 6. Usually, they are more complex and difficult to analyze than non-adaptive systems, but they offer the possibility of substantially increased system performance when input signal characteristics are unknown or time varying.

Linked with adaptive systems, are artificial neural networks or artificial neural network systems. According to Haykin [2], [3], a neural network can be defined as follows: "A neural network consist of the interconnection of a large number of nonlinear processing units called *neurons*; that is, the nonlinearity is distributed throughout the network. We are interested in a particular class of neural networks that *learn* about their environment in a *supervised manner*. We have a desired response that provides a target signal, which the neural network tries to approximate during the learning process – achieved by adapting *synaptic weights*, in a systematic manner." In the context of adaptive signal processing applications, neural networks offer the following advantages [2], [3]: *nonlinearity, input-output mapping, weak statistical assumptions, learning capability, generalization, fault tolerance, and VLSI implementation.*

In this paper, a very brief review of adaptive neural network applications in medical imaging is given. In the next section, the results of literature search on neural

networks in medical imaging are presented, as well as a snapshot of selected applications. In section III, case studies of the application of neural networks in the analysis of cervicovaginal smears, mammography, histopathology, ultrasound imaging of the carotid artery, and in the analysis of physiological data for lesion placement in pallidotomy are presented. Finally, in section IV concluding remarks are presented. This paper shares content with another review paper on data fusion in medical imaging published also in these proceedings [4].

II. Literature review and a snapshot of selected applications

The INSPEC and Medline databases were searched with keywords neural networks and medical imaging, and microscopy, or PET, or SPECT, or CT, or ultrasound, or MRI, or X-ray. The number of papers (including both conference and regular journal papers) published under these categories in the years 1991 to 2000 are given in Fig. 1. There were a total of 542 papers published, with 156 and 386 papers published for the years 1991-95, and 1996-00. These papers cover applications of neural networks for all the physiological systems of the human body, with the majority of them covering the cardiovascular and the nervous systems.

A snapshot of selected applications of neural networks in medical imaging is given in Table I.

III. Case studies

In this section, case studies of medical imaging applications of neural networks in the analysis of cervicovaginal smears, mammography, microscopy, ultrasound imaging, and lesion placement in pallidotomy are presented.

III.I The application of PAPNET in diagnostic cytology [5]-[8]

Diagnostic cytology is a branch of pathology that attempts to diagnose human diseases, mainly cancer or precancerous states of various organs, by microscopic examination of cell samples, rather than tissue biopsies. Cells may be obtained by scraping or brushing the surface of the target organs, such as uterine cervix, or by means of a needle syringe for aspiration of fluids accumulated in a body cavity. The differences between benign and malignant cells are reflected via staining procedures of the nucleus of the cells.

Cytologic techniques serve two different purposes: cancer detection and cancer diagnosis. Consider for example the cervicovaginal smear (Papanicolaou test)

that has for its purpose the discovery of occult precancerous lesions of the uterine cervix. The screening of cervicovaginal smears is a very difficult human task. Smears may be composed of 50,000 to 250,000 normal cells, with at least 90% of the smear specimens being within normal limits. In a recent survey of American laboratories of cytopathology, the false negative error rate reported ranged from 10 to 20% depending on the abnormality. This measure was recorded for women with biopsy-documented neoplastic lesions.

The PAPNET system has been developed for the purpose of selecting a limited number of cells from cytologic preparations for displaying as images in a high-resolution monitor. The system is interactive and does not attempt to render automated diagnostic opinion. The smear is scanned with a low power objective to identify the areas covered by stained nuclei. The cellular areas are reexamined under the medium power objective that performs the first selection of cells based on size and contrast. The selected regions are reanalyzed with a high power objective and two neural nets to identify images of 64 tiles of single or isolated cells, and 64 images of cell clusters. The ANN assigns a high value to abnormal cells, and a low value to negative cells.

The system was tested on 10 cytopathology labs in the US based on rescreening 497 negative cervicovaginal smears from 228 women who developed biopsy-documented high grade precancerous lesions or invasive carcinoma plus control smears from each laboratory. PAPNET revealed abnormalities that would have led to earlier discovery and treatment of these patients. From the 9666 negative control smears, 127 precancerous lesions were discovered (1.3%). The PAPNET system was approved as a quality control instrument for cervical smears by the FDA.

III.II Computer-Aided Diagnosis in Mammography [9]-[13]

Breast cancer is the most common malignancy in women and the second most common cause of death from malignancy in this population. In US, more than 180,000 women develop the disease each year. The practice of mammography is regulated in US through the FDA Mammography Quality of Standards Act 92. It is estimated that over 100 groups are working for the detection or characterization of masses and clustered microcalcifications in digital mammography.

Radiographically, mass lesions can be characterised by their degree of spiculation, margin definition, shape, and texture (density, homogeneity). In addition, clustered microcalcifications can be characterized by the morphology of individual calcification, e.g. shape, area, brightness, the heterogeneity of individual features

within a cluster, and their spatial distribution. The Department of Radiology at the University of Chicago, developed a CAD system in mammography based on the above mentioned features. Selected features were inputted to an artificial neural network that was trained to compute the percentage of malignancy of suspected lesions. This system, named ImageChecker M1000 was made commercially available by R2 Technology, Inc., Los Altos, California. A large study involving a retrospective analysis of 1083 consecutive cancer cases from 13 institutions and more than 24 radiologists was performed as part of the FDA approval process for the ImageChecker M1000. The sensitivity was 98.3% for microcalcification cluster detection and 72% for mass detection with an average false-positive rate of one per image. A prospective component of their study included an analysis of 14,817 cases with the CAD system. No statistically significant change was observed in the radiologists' workup rate when the system was used as an aid in the screening setting. A second commercial mammography CAD system, SecondLook from Qualia and Scanis, is also seeking FDA approval. Finally, it is noted that in mammographic CAD, the CAD system is used for providing a second opinion and not as a standalone system, and hence need not be perfect.

III.III A Modular Neural Network System for the Analysis of Nuclei in Histopathological Sections [14]-[17]

The evaluation of immunocytochemically stained histopathological sections presents a complex problem due to many variations that are inherent in the methodology. This subsection describes a modular neural network system that is being used for the detection and classification of breast cancer nuclei named Biopsy Analysis Support System (BASS). The system is based on a modular architecture where the detection and classification stages are independent. Two different methods for the detection of nuclei are being used: the one approach is based on a feed forward neural network (FNN) which uses a block-based singular value decomposition (SVD) of the image, to signal the likelihood of occurrence of nuclei. The other approach consists of a combination of a receptive field filter and a squashing function (RFS), adapting to local image statistics to decide on the presence of nuclei at any particular image location. The classification module of the system is based on a radial basis function neural network. A total of 57 images captured from 41 biopsy slides containing over 8300 nuclei were individually and independently marked by two experts. A five scale grading system, known as diagnostic index, was used to classify the nuclei staining intensities. The experts' mutual detection sensitivity (SS) and positive predictive value (PPV) were found to be 79% and 77%

respectively. The overall joint performance of the FNN and RFS modules were 55% for SS and 82% for PPV. The classification module correctly classified 76% of all nuclei in an independent validation set containing 25 images. In conclusion, this study shows that the BASS system simulates the detection and grading strategies of human experts and it will enable the formulation of more efficient standardization criteria, which will in turn improve the assessment accuracy of histopathological sections.

III.IV A Multi-feature Multi-classifier System for the Classification of Atherosclerotic Carotid Plaques [18]-[20]

There are indications that the morphology of atherosclerotic carotid plaques, obtained by high-resolution ultrasound imaging, has prognostic implications. The objective of this work was to develop a computer-aided system that will facilitate the characterisation of carotid plaques for the identification of individuals with asymptomatic carotid stenosis at risk of stroke. A total of 230 plaque images were collected which were classified into two types: symptomatic because of ipsilateral hemispheric symptoms, or asymptomatic because they were not connected with ipsilateral hemispheric events. Ten different texture feature sets were extracted from the manually segmented plaque images using the following algorithms: first order statistics, spatial gray level dependence matrices, gray level difference statistics, neighbourhood gray tone difference matrix, statistical feature matrix, Laws texture energy measures, fractal dimension texture analysis, Fourier power spectrum and shape parameters. For the classification task a modular neural network composed of self-organizing map (SOM) classifiers, and combining techniques based on a confidence measure were used. Combining the classification results of the ten SOM classifiers inputted with the ten feature sets improved the classification rate of the individual classifiers, reaching an average diagnostic yield of 73.1%. The same modular system was implemented using the statistical k-nearest neighbour (KNN) classifier. The combined diagnostic yield for the KNN system was 68.8%. The results of this work show that it is possible to identify a group of patients at risk of stroke based on texture features extracted from ultrasound images of carotid plaques. This group of patients can benefit from a carotid endarterectomy whereas other patients will be spared from an unnecessary operation

III.V Neural Network Analysis of Physiological Data for Lesion Placement in Pallidotomy [21]-[23]

Current pharmacological therapy for Parkinson's disease loses its usefulness over time. Recently, pallidotomy, a surgical treatment for many of the symptoms of Parkinson's, has been re-investigated. This procedure requires localization of a small region within the globus pallidus. In this work, a simple electrophysiological analysis, used in conjunction with MRI imaging, provides excellent localization of the target derived from imaging studies alone. Investigation of more complex mathematical analysis may yield additional tools for localization. A new feature in this research is the after-lesioning recordings. It has been proven to be valuable in re-assessing the condition of the patient. If residual activity is observed at the after-lesioning recording "session", additional lesions might be made, which might further alleviate the Parkinson symptoms.

IV. Concluding Remarks

Concluding remarks are organized under two main categories: medical imaging issues in general, and adaptive neural networks. For the former, the following remarks are made, motivated by Duncan and Ayche [24]:

1. Work in general must be developed and clearly motivated. Analysis should target both normal and pathology cases.

2. Medical image analysis tasks are taken in isolation, rather than considered together, i.e. segmentation and registration are pieces of the same underlying task of identifying structure.

3. Need to develop appropriate validation and evaluation approaches. There is also, lack of availability of test data sets. Need for the formation of common datasets where algorithms can be compared and contrasted to.

4. The medical image analysis community must interact more with other communities, especially the medical physics community.

Some concluding remarks about adaptive neural network applications in medical systems are given for future researchers (see also [25]):

1. Clarify the purpose of the study.
2. Validate your results appropriately.
3. Benchmark against a suitable alternative.

4. Develop critical trials involving the exercise of human judgment. Concluding, adaptive neural network applications in medical imaging need to be incorporated into CAD systems, including clinical data, thus enabling the early diagnosis, disease monitoring, better patient treatment, and the offering of a better service to the citizen.

Table I A snapshot of selected applications of neural networks in medical imaging

X-ray [26][27]	CT [28][29]
MRI [30][31]	Ultrasound [32][33]
Nuclear Medicine [34]	Microscopy [35]

References

- [1] B. Widrow, and S.D. Stearns, *Adaptive Signal Processing*, Prentice Hall, 1985.
- [2] S. Haykin, *Adaptive Filter Theory*, 3rd ed, Prentice Hall, 1996.
- [3] S. Haykin, *Neural Networks*, 2nd ed., Prentice Hall, 1999.
- [4] C.S. Pattichis, M.S. Pattichis, and E. Micheli-Tzanakou, "Medical imaging fusion applications: An overview," *Proc. the 35th Asilomar Conf. on Signals, Systems, and Computers*, 2001.
- [5] L.G. Koss, "The application of PAPNET to diagnostic cytology," in *Artificial Neural Networks in Biomedicine*, P.G. Lisboa, E.C. Ifeachor, and P.S. Szczepaniak Eds, Springer, 2000, pp. 51-67.
- [6] L.J. Mango, "Computer-assisted cervical cancer screening using neural network," *Cancer Letters*, vol. 77, pp. 155-162, 1994.
- [7] L.G. Koss, E. Lin, K. Schreiber, P. Elgert, and L. Mango, "Evaluation of the PAPNET cytologic screening system for quality control of cervical smears," *Am. J. Clin. Path.*, vol. 101, pp. 220-229, 1994.
- [8] L.G. Koss, et. al., "Significant reduction in the rate of false-negative cervical smears with neural network-based technology PAPNET system," *Human Path.*, vol. 7, pp. 1196-1203, 1997.
- [9] M.L. Giger, Z. Huo, M.A. Kupinski, C.J. Vyborny, "Computer-Aided Diagnosis in Mammography," in *Handbook of Medical Imaging Vol. 2 Medical Image Processing and Analysis*, M. Sonka, and J.M. Fitzpatrick (Eds), SPIE Press, 2000, pp. 915-1004.
- [10] Y. Wu, et al., "Application of neural networks in mammography," *Radiology*, vol. 187, pp. 81-87, 1993.
- [11] Z. Huo, et al., "Effect of dominant features on neural network performance in the classification of mammographic lesions," *Phys. Med. Biol.*, vol. 44, pp. 2579-2595, 1999.
- [12] M.A. Kupinski and M.A. Anastasio, "Multiobjective genetic optimization of diagnostic classifiers with implications for generating receiver operating characteristic curves," *IEEE Trans. Med. Imaging*, vol. 18, pp. 675-685, 1999.
- [13] J. Roehrig, T. Doi, A. Hasegawa, B. Hunt, et. al., "Clinical results with r2 imagechecker system," in *Digital Mammography 1998*, Dordrecht, The Netherlands), Kluwer Academic Publishers, 1998, pp. 395-400.
- [14] F. Schnorrenberg, C.S. Pattichis, et al., "Computer-aided Classification of Breast Cancer Nuclei," *Technology and Health Care*, vol. 4, no. 2, pp. 147-161, 1996.
- [15] F. Schnorrenberg, C.S. Pattichis, K.C. Kyriacou, and C.N. Schizas, "Computer-Aided Detection of Breast Cancer Nuclei," *IEEE Trans. Inf. Tech. Biom.*, vol. 1, no. 2, pp. 128-140, 1997.
- [16] F.S. Schnorrenberg, N. Tsapatsoulis, C.S. Pattichis, C.N. Schizas, S. Kollias, M. Vassiliou, A. Adamou, and K. Kyriacou, "Improved Detection of Breast Cancer Nuclei Using Modular Neural Networks," *IEEE Eng. in Med. and Biol.*

Mag., Special Issue on Classifying Patterns with Neural Networks, vol. 19, no. 1, pp. 48-63, 2000.

[17] F. Schnorrenberg, C.S. Pattichis, et al., "Content-based Retrieval of Breast Cancer Biopsy Slides," *Technology and Health Care*, vol. 8, pp. 291-297, 2000.

[18] C.I. Christodoulou, C.S. Pattichis, M. Pantziaris, T. Tegos, A. Nicolaides, T. Elatrozy, M. Sabetai, and S. Dhanjil, "Multi-feature texture analysis for the classification of carotid plaques," in *CD-ROM Proc. of the Int. Joint Conf. on Neural Networks, IJCNN '99*, Washington DC, 10-16 July, 1999.

[19] C.I. Christodoulou, and C.S. Pattichis, "Medical diagnostic systems using ensembles of neural SOFM classifier," in *Proc of the 6th IEEE Int. Conf. on Electronics, Circuits and Systems, ICECS '99*, Paphos, Cyprus, Sept. 5-8, 1999, vol. 1, pp. 109-112.

[20] C.I. Christodoulou, C.S. Pattichis, M. Pantziaris, and A. Nicolaides, "Texture based classification of atherosclerotic carotid plaques," submitted to *IEEE Trans. Med. Imag.*, revised version in Nov. 2001.

[21] R.M. Lehman, E. Micheli-Tzanakou, Jian Zheng and J.L. Hamilton, "Electrophysiological recordings in pallidotomy localized to 3D stereoscopic imaging" *Stereotactic and Functional Neurosurgery*, vol. 72, pp. 185-191, 1999.

[22] R.M. Lehman, Jian Zheng, J. Hamilton, and E. Micheli-Tzanakou, "Comparison of 3-D- MR imaging with pre and post lesion recording in pallidotomy", *Acta Neurochirurgica*, vol. 142, pp. 319-328, 2000.

[23] R. M. Lehman, E. Micheli-Tzanakou, et al., "Quantitative on-line analysis of physiological data for lesion placement in pallidotomy", *Neurosurgery*, vol 729, pp. 1-15, 2001.

[24] J.S. Duncan, and N. Ayache, "Medical image analysis: Progress over two decades and the challenges ahead," *IEEE Trans. PAMI*, vol. 22, no. 1, pp. 85-102, 2000.

[25] P.J.G. Lisboa, "A review of evidence of healthcare improvements involving the application of artificial neural networks," in *Proc. of the 4th Int. Conf. On Neural Networks and Expert Systems in Medicine and Healthcare*, G.M. Papadourakis, Ed., Greece, pp. 3-10, 2001.

[26] Yu Songyang, and G. Ling, "A CAD system for the automatic detection of clustered microcalcifications in digitized mammogram films," *IEEE Trans. on Med. Imag.*, vol. 19, no.2, pp. 115-126, 2000.

[27] J. Duryea, Y. Jiang, M. Zakharevich, H.K. Genant, "Neural network based algorithm to quantify joint space width in joints of the hand for arthritis assessment," *Medical Physics*, vol. 27, no.5, pp. 1185-1194, 2000.

[28] J.E. Koss, et al., "Abdominal organ segmentation using texture transforms and a Hopfield neural network," *IEEE Trans. on Med. Imag.*, vol. 18, no.7, pp. 640-648, 1999.

[29] C. E-Liang, et al., "An automatic diagnostic system for CT liver image classification," *IEEE Trans. on Biom. Eng.*, vol. 45, no. 6, pp.783-794, 1999.

[30] C. Kai-Hsiang, et al. "Model-free functional MRI analysis using Kohonen clustering neural network and fuzzy C-means," *IEEE Trans. Med. Imag.*, vol. 18, no. 12, pp. 1117-1128, 1999.

[31] S. Banerjee, and D. Majumdar, "Shape matching in multimodal medical images using point landmarks with Hopfield net," *Neurocomputing*, vol. 30, no. 1-4, pp. 103-116.

[32] T. Yen-Hao, et al., "3-D heart modeling and motion estimation based on continuous distance transform neural networks and affine transform," *J. VLSI Sig. Proc. Systems for Sig., Im., and Video Techn.*, vol. 18, no. 3, pp. 207-218, 1998.

[33] Y.M. Kadah, "Classification algorithms for quantitative tissue characterization of diffuse liver disease from ultrasound images," *IEEE Trans. Med. Imag.*, vol. 15, no. 4, pp. 466-478, 1996.

[34] L.J. Sung, et al., "Localization of epileptogenic zones in F-18 FDG brain PET of patients with temporal lobe epilepsy using artificial neural network," *IEEE Trans. Med. Imag.*, vol. 19, no. 4, pp. 347-355, 2000.

[35] M.S. Beksac, S. Eskiizmirli, A.N. Cakar, A.M. Erkmen, A. Dagdeviren, and C. Lundsteen, "An expert diagnostic system based on neural networks and image analysis techniques in the field of automated cytogenetics," *Technology and Health Care*, vol. 3, no.4, pp.217-29, 1996.

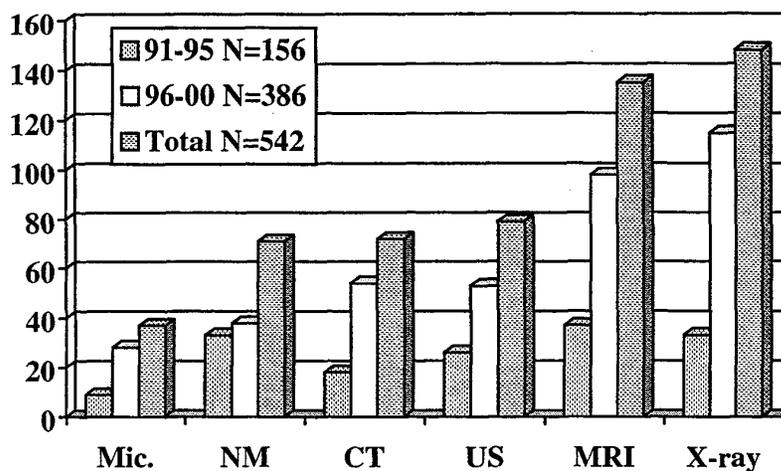


Fig. 1 Results of the INSPEC and Medline databases search with keywords neural networks and medical imaging, and microscopy (mic.), or PET, or SPECT (NM for nuclear medicine is given), or CT, or ultrasound (US), or MRI, or X-ray. For each entry, the first, second, and third bars show the hits for the periods 91-95, 96-00, and their sum respectively.